

SWE-CX63

Brightfield Microscope

Automatic Brightness Adjustment Panel



Widely used for observing and analyzing the fine structures and characteristics of biological samples




SWE-CX63

Issue: During batch imaging of tissue sections, significant background brightness variations render images unusable.

The exclusive Brightness Following (LIM Light Intensity Management) feature, work with software, memorizes photography brightness and exposure time to ensure the accuracy and consistency of experimental data.

Auto-Adjusted Illumination

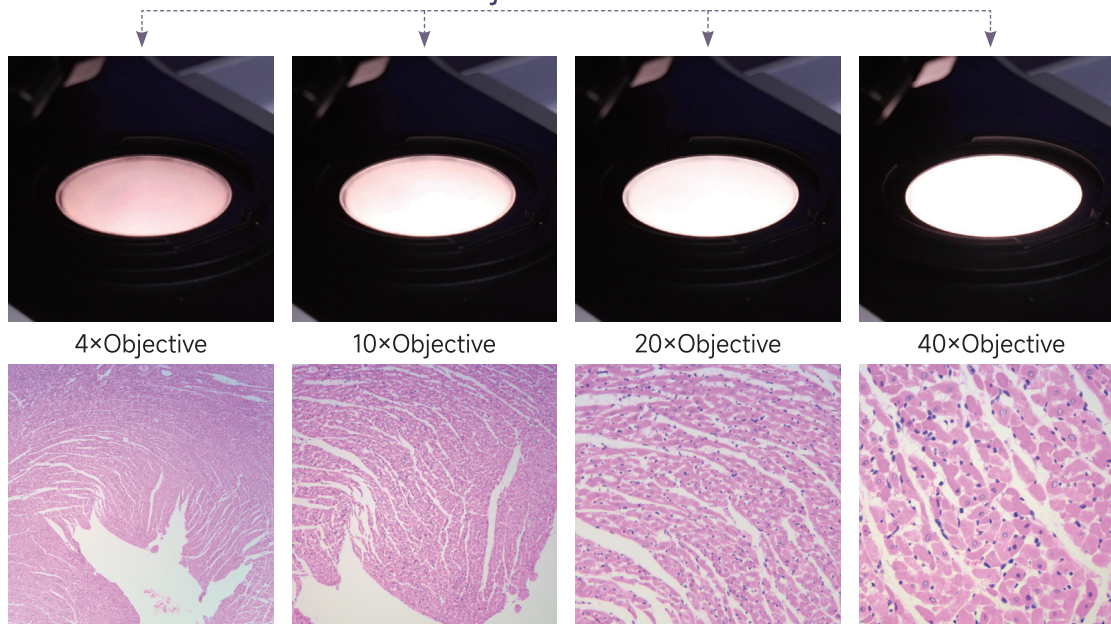


SWE-CX63

Issue: Manuscript rejection due to missing/dimisscaled scale bars in section images.

Imaging software automatically detects objective magnification and applies the correct scale bar.

Automatic synchronization of objective magnification

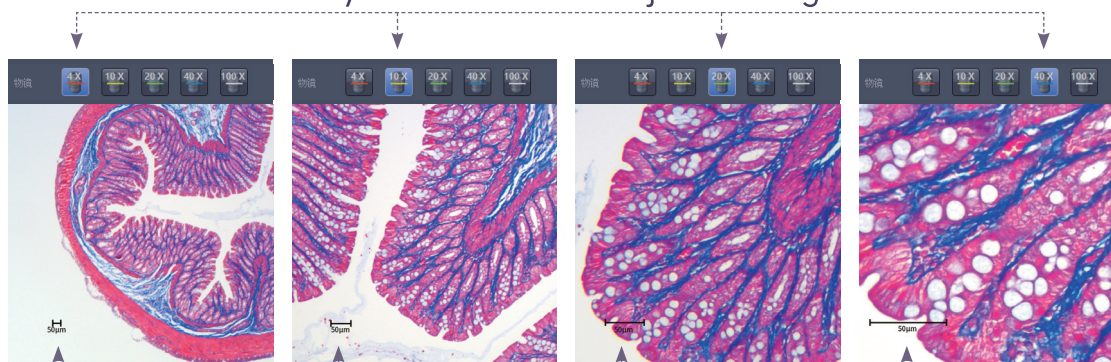

Auto-Updated Scale Bar